


GC CAPILLARY COLUMN APPLICATIONS: CLINICAL/TOXOLOGICAL

Mace

Column: 007-17, (50% Phenyl)
Methylpolysiloxane
25M. x 0.25mm I.D. x
0.25µm film
Cat. No.: 007-17-25-0.25F
Temperature: 100° (1 min. hold)
(10°/min.) -280°C
Injector: 220°C
Detector: MSD
Carrier Gas: 28 cm/sec., Helium

1. 2-Chloroacetophenone
2. contaminant
3. contaminant
4. o-Chlorobenzalmononitrile

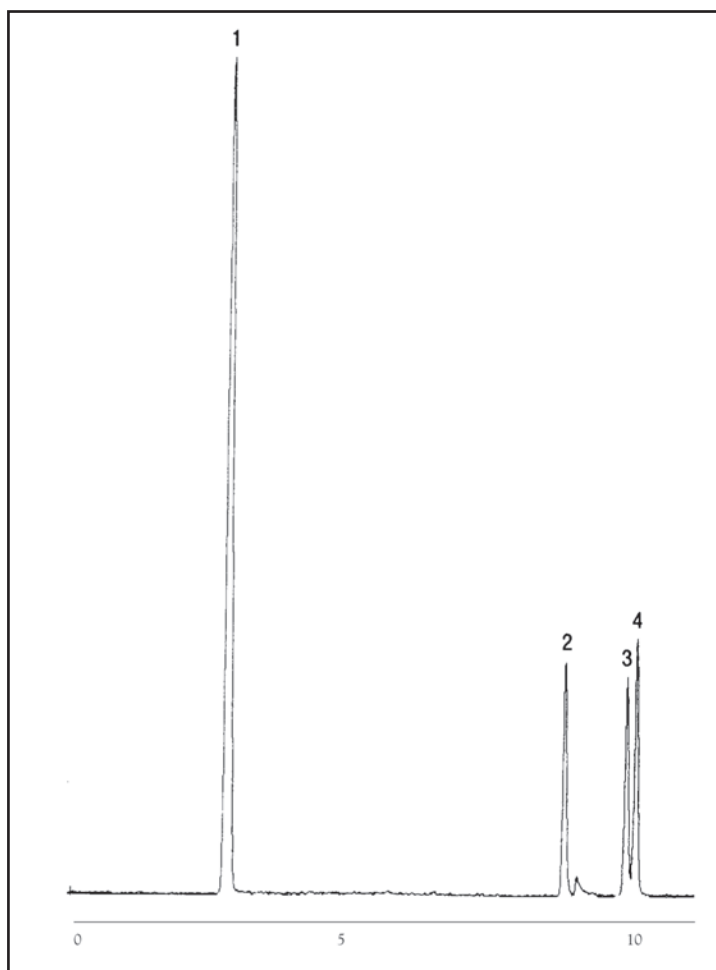

PO Box 3881, Woodbridge, CT 06525 • (203) 393-3112 • FAX (203) 393-0391
TOLLFREE: 800-275-7033 • E-MAIL: tech@quadrexcorp.com